


Amaxa[®] Cell Line 96-well Nucleofector[®] Kit SF


For SH-SY5Y

Human neuroblastoma; adherent epithelial cells

Example for Nucleofection[®] of SH-SY5Y cells

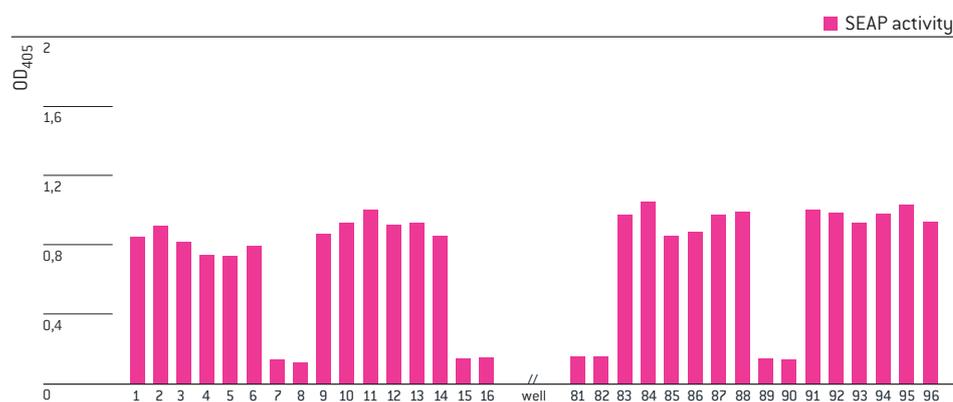

Well-to-well uniformity of reporter gene expression after 96-well Nucleofection[®] of SH-SY5Y cells. SH-SY5Y cells were transfected with 0.4 µg of a plasmid encoding a secreted version of human placental alkaline phosphatase (SEAP) using the Cell Line 96-well Nucleofector[®] Kit SF. 24 hours post Nucleofection[®], alkaline phosphatase activity of cell culture supernatants was measured (n = 72, SD ± 12% from the mean). Wells without SEAP enzyme activity are negative controls of cells in 96-well Nucleofector[®] Solution and plasmid DNA, but without Nucleofection[®].

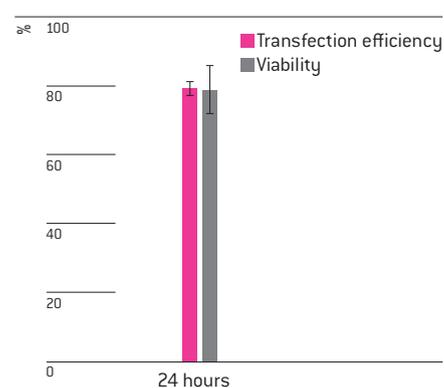

Transfection efficiency of SH-SY5Y cells 24 hours post Nucleofection[®]. 2 x 10⁵ SH-SY5Y cells were transfected with program 96-CA-137 and 0.4 µg of pmaxGFP[®] Vector. 24 hours post Nucleofection[®] cells were analyzed on a FACSCalibur[™] with HTS option [Becton Dickinson]. Cell viability (CellTiter-Blue[®] cell viability assay) is approximately around 80% after 24 hours.

Product Description

Cat. No.	VHCA-1002	VHCA-2002
Size (reactions)	1 x 96	10 x 96
Cell Line 96-well Nucleofector [®] Solution SF	2.025 ml	20.25 ml
Supplement	0.45 ml	4.5 ml
pmaxGFP [®] Vector (0.2 µg/µl in 10 mM Tris pH 8.0)	45 µg	45 µg
Nucleocuvette [®] Plate(s)	1	10
Storage and stability	Store Nucleofector [®] Solution, Supplement and pmaxGFP [®] Vector at 4°C. For long-term storage, pmaxGFP [®] Vector is ideally stored at -20°C. The expiration date is printed on the solution box. Once the Nucleofector [®] Supplement is added to the Nucleofector [®] Solution, it is stable for three months at 4°C.	

Note 96-well Nucleofector[®] Solutions and standard Nucleofector[®] Solutions are not compatible.

Required Material

Note Please make sure that the entire supplement is added to the Nucleofector® Solution.

- Nucleofector® 96-well Shuttle System (Nucleofector® Device, version IIS; 96-well Shuttle® Device; laptop with 96-well Shuttle® Software)
- Supplemented 96-well Nucleofector® Solution at room temperature
- Supplied Nucleocuvette® Plate(s)
- Supplied pmaxGFP® Vector
- Substrate of interest, highly purified, preferably by using endotoxin-free kits; A260 : A280 ratio should be at least 1.8
- Nucleocuvette® compatible tips: epT.I.P.S. [US/CDN: Eppendorf North America, Cat. No. 2491.431, Rest of World: Eppendorf AG, Cat. No. 0030073.266], Matrix TallTips® [Matrix Technologies Corp., Cat. No. 7281] or LTS Tips [Rainin Instrument, LLC, Cat. No. SR-L10F, SR/SS-L250S, SR/SS-L300S]. Before using other types of pipette tips, please ensure they reach the bottom of the Nucleocuvette® Wells without getting stuck
- 96-well culture plates or culture plates of your choice
- **For detaching cells:** 0.5 mg/ml Trypsin and 0.2 mg/ml EDTA in PBS and supplemented culture media or PBS/0.5% BSA
- **Culture medium:** 1 : 1 mixture of EMEM and Ham's F12 Nutrient-Mixture [Lonza, Cat. No.: 12-615F] supplemented with 10% FCS and 1% Penicilin/Streptomycin
- Prewarm appropriate volume of culture medium to 37°C (255 µl per sample)
- Appropriate number of cells (2 x 10⁵ cells per sample; lower or higher cell numbers may influence transfection results)

1. Pre Nucleofection®

Cell culture recommendations

- 1.1 Thaw SH-SY5Y cells and transfer them into culture medium
- 1.2 Passage cells every 2 – 3 days. We recommend using cells maximally to passage 14
- 1.3 Seed out 5 x 10⁶ cells/T75 flask
- 1.4 Subculture 3 days before Nucleofection®

Trypsinization

- 1.5 Remove media from the cultured cells and wash cells once with PBS ; use at least same volume of PBS as culture media
- 1.6 For harvesting, incubate the cells ~5 minutes at 37°C with indicated trypsinization reagent (please see required material)
- 1.7 Neutralize trypsinization reaction with supplemented culture medium or PBS/0.5% BSA once the majority of the cells (>90%) have been detached

2. Nucleofection®

One Nucleofection® Sample contains

2 x 10⁵ cells

0.4 – 0.8 µg plasmid DNA (in 1 – 2 µl H₂O or TE) or 0.4 µg pmaxGFP® Vector or 30 - 300nM siRNA
(0.6 – 6 pmol/sample)

20 µl Cell Line 96-well Nucleofector® Solution SF

- 2.1 Please make sure that the entire supplement is added to the Nucleofector® Solution
- 2.2 Start Nucleofector® 96-well Shuttle® Software, verify device connection and upload experimental parameter file (for details see device and software manuals)
- 2.3 Select the appropriate 96-well Nucleofector® Program **96-CA-137**
- 2.4 Prepare cell culture plates by filling appropriate number of wells with desired volume of recommended culture media, e.g. 175 µl* (see note at the end of this chapter) for one well of a 96-well plate and pre-incubate/equilibrate plates in a humidified 37°C/5% CO₂ incubator
- 2.5 Pre-warm an aliquot of culture medium to 37°C (80 µl per sample*)
- 2.6 Prepare **0.4 – 0.8 µg plasmid DNA** or 0.4 µg pmaxGFP® Vector or **30 nM – 300 nM siRNA** (0.6 – 6 pmol/sample)
- 2.7 Harvest the cells by trypsinization (please see 1.5 – 1.7)
- 2.8 Count an aliquot of the cells and determine cell density
- 2.9 Centrifuge the required number of cells (**2 x 10⁵ cells per sample**) at **90xg for 10 minutes** at room temperature. Remove supernatant completely
- 2.10 Resuspend the cell pellet carefully in 20 µl room temperature 96-well Nucleofector® Solution per sample

A. One or several substrates (DNAs or RNAs) in multiples:

- Prepare mastermixes by dividing cell suspension according to number of substrates
- Add required amount of substrates to each aliquot (max. 2 µl per sample)
- Transfer 20 µl of mastermixes into the wells of the 96-well Nucleocuvette® Modules

B. Multiple substrates (e.g. library transfection):

- Pipette 20 µl of cell suspension into each well of a sterile U- or V-bottom 96-well microtiter plate
- Add 2 µl substrates (maximum) to each well
- Transfer 20 µl of cells with substrates into the wells of the 96-well Nucleocuvette® Modules

Note It is advisable to pre-dispense each cell suspension into a sterile round-bottom 96-well plate or to pipet from a pipetting reservoir for multi-channel pipettes. Use a multi-channel or single-channel pipette with suitable pipette tips. As leaving cells in 96-well Nucleofector® Solution for extended periods of time may lead to reduced transfection efficiency and viability it is important to work as quickly as possible. Avoid air bubbles while pipetting.

- 2.11 Gently tap the Nucleocuvette® Plate to make sure the sample covers the bottom of the well
- 2.12 Place 96-well Nucleocuvette® Plate with closed lid into the retainer of the 96-well Shuttle. Well “A1” must be in upper left position

- 2.13 Start 96-well Nucleofection® Process by either pressing “Upload and start” in the 96-well Shuttle® Software or pressing “Upload” in the 96-well Shuttle® Software and then the “Start” button at the 96-well Shuttle® (for both options please refer to the respective Manual)
- 2.14 After run completion, open retainer and carefully remove the 96-well Nucleocuvette® Plate from the retainer
- 2.15 Incubate Nucleocuvette® Plate for 10 minutes at room temperature
- 2.16 Resuspend cells with 80 µl* (recommendation for 96-well plates) or desired volume of pre-warmed medium (maximum cuvette volume 200 µl). Mix cells by gently pipetting up and down two to three times
- 2.17 Plate desired amount of cells in culture system of your choice. Recommendation for 96-well plates: Transfer 25 µl of resuspended cells to 175 µl pre-warmed medium prepared in 96-well culture plates*

*** Note** The indicated cell numbers and volumes have been found to produce optimal 96-well Nucleofection® Results in most cases. However, depending on your specific needs you may wish to test an extended range of cell numbers. Cell numbers and volumes can be adapted such that fewer cells are transferred or duplicate plates can be seeded.

3. Post Nucleofection®

- 3.1 Incubate the cells in humidified 37°C/5% CO₂ incubator until analysis. Gene expression or down regulation, respectively, is often detectable after only 4 – 8 hours

Additional Information

For an up-to-date list of all Nucleofector® References, please refer to:
www.lonza.com/nucleofection-citations

For more technical assistance, contact our Scientific Support Team:

USA/Canada
Phone: 800 521 0390 (toll-free)
Fax: 301 845 8338
E-mail: scientific.support@lonza.com

Europe and Rest of World
Phone: +49 221 99199 400
Fax: +49 221 99199 499
E-mail: scientific.support.eu@lonza.com

Lonza Cologne AG
50829 Cologne, Germany

Please note that the Amaxa® Nucleofector® Technology is not intended to be used for diagnostic purposes or for testing or treatment in humans.

The Nucleofector® Technology, comprising Nucleofection® Process, Nucleofector® Device, Nucleofector® Solutions, Nucleofector® 96-well Shuttle® System and 96-well Nucleocuvette® plates and modules is covered by patent and/or patent-pending rights owned by Lonza Cologne AG.

Amaxa, Nucleofector, Nucleofection, 96-well Shuttle, Nucleocuvette and maxGFP are either registered trademarks or trademarks of the Lonza Cologne AG in Germany and/or U.S. and/or other countries.

Other product and company names mentioned herein are the trademarks of their respective owners.

This kit contains a proprietary nucleic acid coding for a proprietary copepod fluorescent protein intended to be used as a positive control with this Lonza product only. Any use of the proprietary nucleic acid or protein other than as a positive control with this Lonza product is strictly prohibited. USE IN ANY OTHER APPLICATION REQUIRES A LICENSE FROM EVROGEN. To obtain such a license, please contact Evrogen at license@evrogen.com.

The CMV promoter is covered under U.S. Patents 5,168,062 and 5,385,839 and its use is permitted for research purposes only. Any other use of the CMV promoter requires a license from the University of Iowa Research Foundation, 214 Technology Innovation Center, Iowa City, IA 52242.

The use of this product in conjunction with materials or methods of third parties may require a license by a third party. User shall be fully responsible for determining whether and from which third party it requires such license and for the obtainment of such license.

No statement is intended or should be construed as a recommendation to infringe any existing patent.

© Copyright 2009, Lonza Cologne AG. All rights reserved DCSF-1008 07/09